



Temperature Control: >1.5K Controlling on Sample with Sorb at 17K

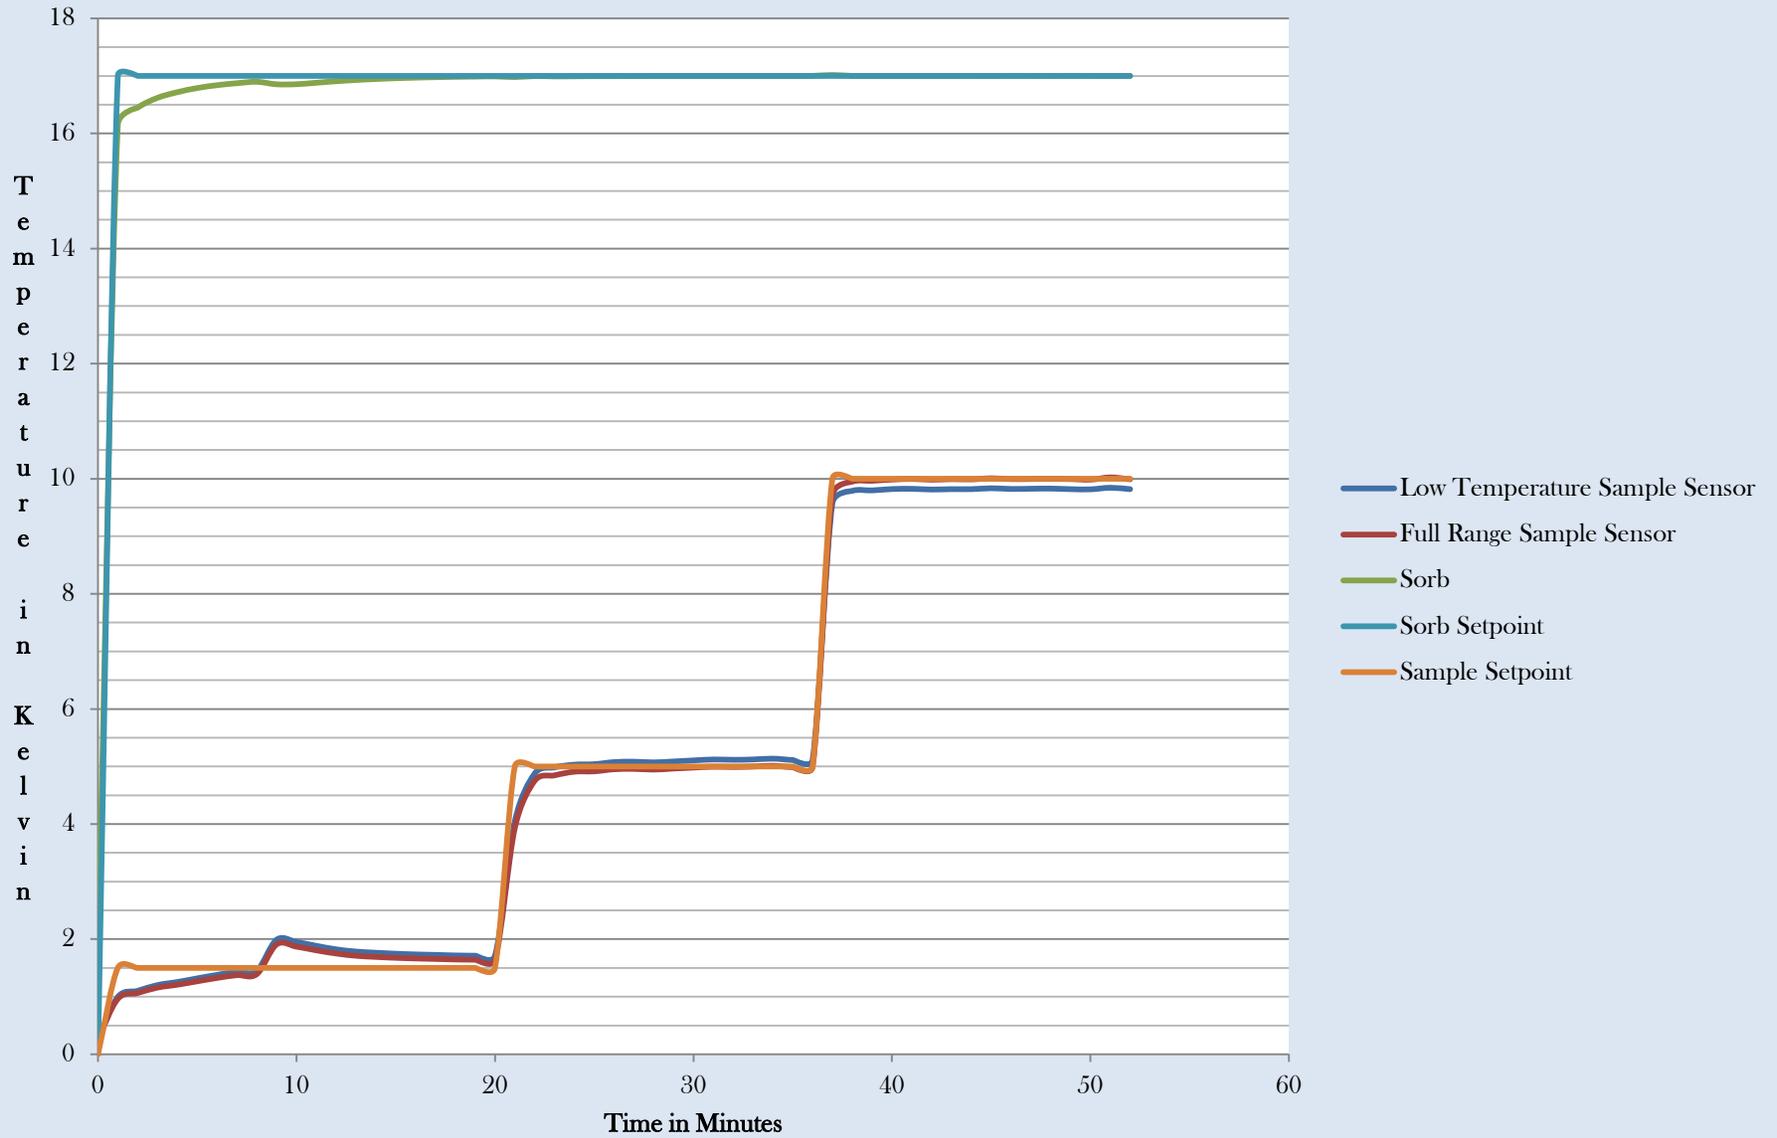

Temperature Control: <1.5K Controlling on Sorb

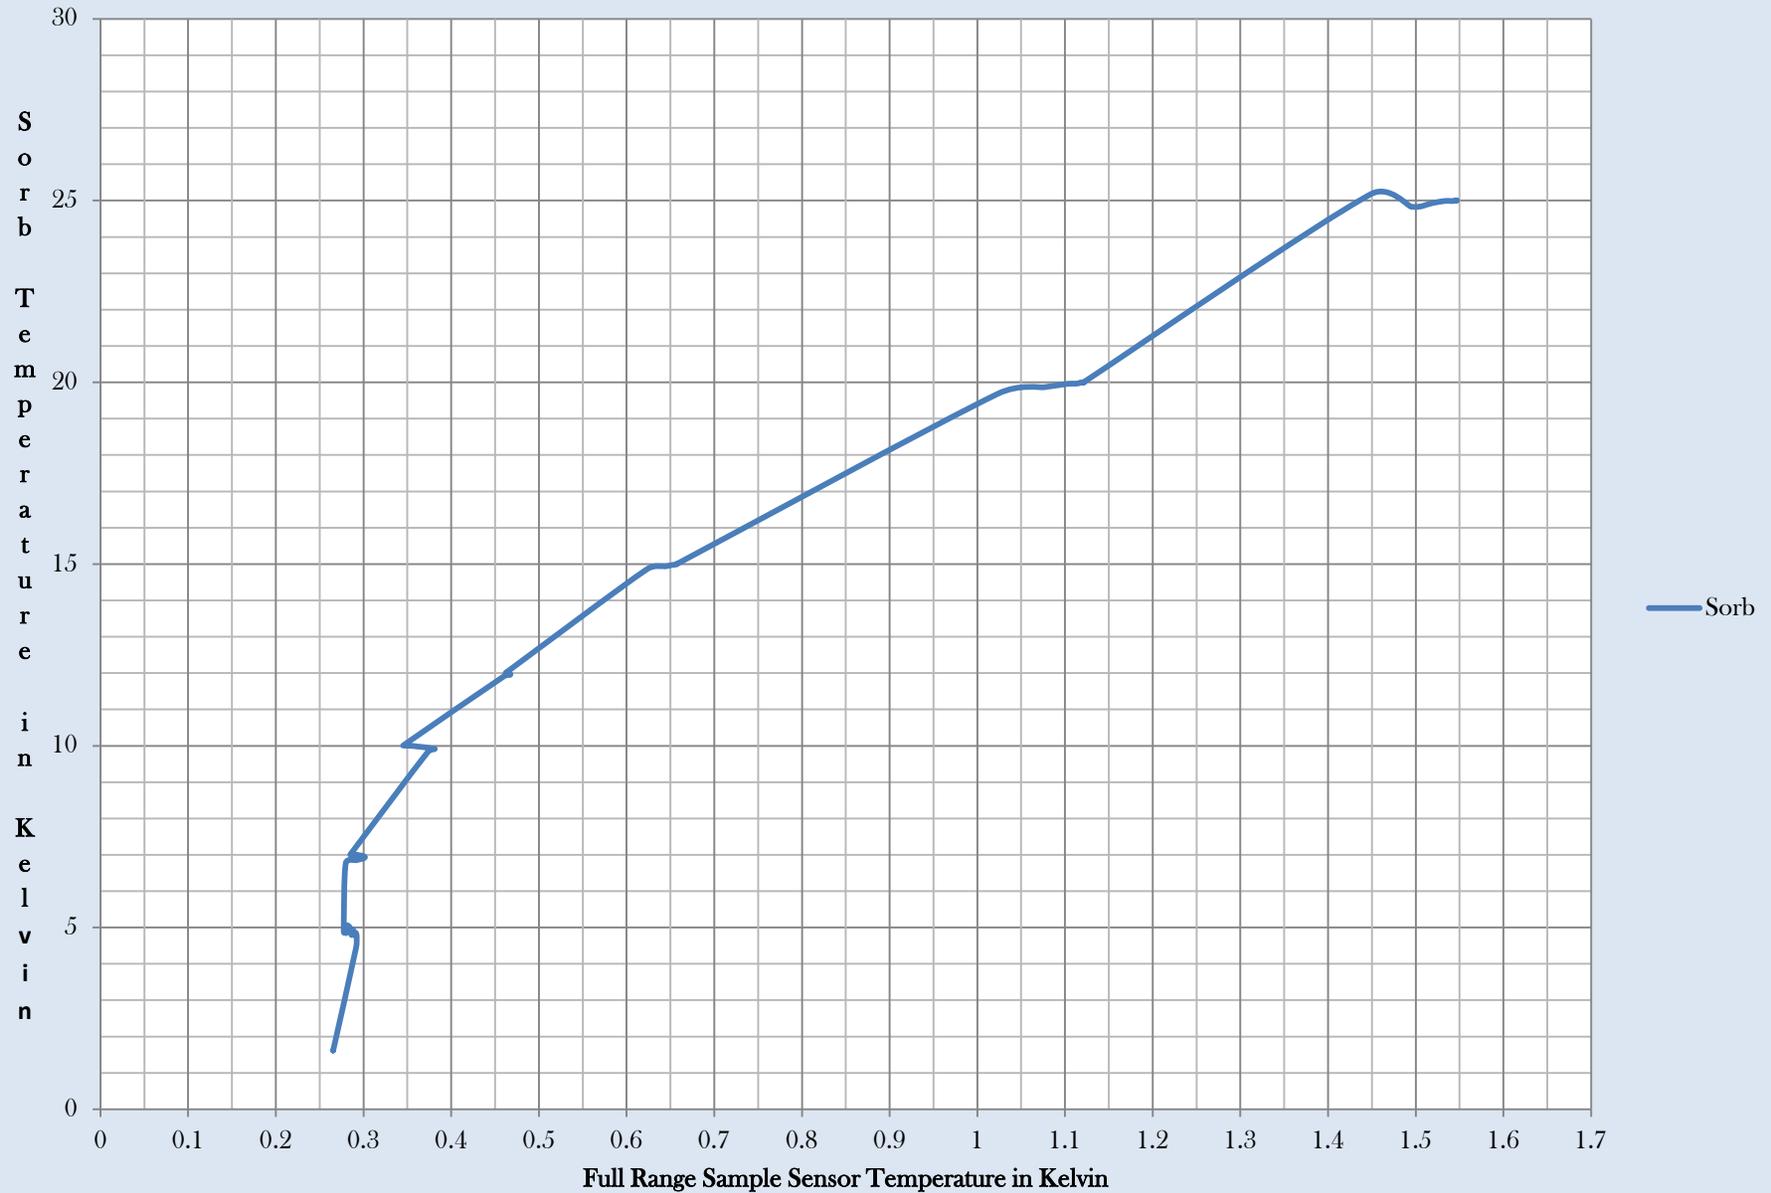

ULT-G Full Range Sample Sensor Control Test 5-8-2015

